



United Testing Corporation (Shanghai)




Query coding: H22440



Job No: 2020-P00338B

Test Report

page 1 of 2

Sample Name	Single-use face mask	Specification	/	Test Type	Commission Test
Sampling site	/	Sample Grade	/	Brand	/
Style	/				
Consigned Unit	Shanghai OGO Medical Instrument Co.,Ltd.				
Manufacturing unit	Shanghai OGO Medical Instrument Co.,Ltd.				
Sample description	BL/WH				
Task source	/	Sample list No	/	Sampling date	/
Quantity	/	number	/	Date Received	2020-3-2
Sample Number	Forty-five	Sampling quantity	/	Date of manufacture	/
Date Received	2020-3-2	Inspection Date	2020-03-02 To 2020-03-16		
Performance Standard	GB/T32610-2016 《Technical specification of daily protective mask》				
Conclusion	 Please see Collection of test results. (Dedicated Inspection Stamp) 160920341338 Date Issued: 2020-03-02				
Consigned Unit	Address	/			
	Zip Code	/	Telephone	/	
Remark					



Approved By:

李平

Checked By:

张怡

Tested By:

刘钦



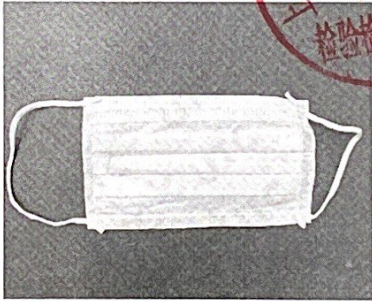
United Testing Corporation (Shanghai)

Test Report

Job No: 2020-P00338B

Sample: Single-use face mask

第 2 页 共 2 页

Test Result						
No.	Items		Unit	Requirement	Result	Judgement
1.	Filter efficiency	Nacl	%	≥95	min: 95.4	Meet
		Paraffin oil	%	≥95	min: 95.1	Meet
2.	Particle protective performance		%	≥90	min: 90.3	Meet
3	Total bacterial count		CFU/g	≤200	<20	Meet
4	Fungus		CFU/g	≤100	Not detected	Meet
5	Coliform bacteria		/	None detected	Not detected	Meet
6	Pseudomonas aeruginosa		/	None detected	Not detected	Meet
7	Staphylococcus aureus		/	None detected	Not detected	Meet
8	Hemolyticstreptococcus		/	None detected	Not detected	Meet
备注	Particle protective performance: A grade, Filter efficiency: Igrade *Subcontract project					
Blank below						
						

技术有限公司
章

